CERTIFICATE OF ANALYSIS

PuriLab Analytical

Bacteriostatic Water 10 mL

BAC-2026-007 Lot IP261001 Analyzed October 12, 2026

TIMELINE

ORDERED
October 9, 2026

RECEIVED
October 12, 2026

ANALYZED
October 12, 2026

SAMPLE

NAME
Bacteriostatic Water 10 mL

EXPECTED
Benzyl Alcohol (preservative)

AMOUNT
1 vial, aqueous solution, multi-dose 10 mL, sealed

TESTING

CLIENT
Investigate Peptides

TEST TYPE
Preservative identity & content determination

METHOD
HPLC-UV

CONTENT, HOW MUCH IS IN IT

0.98% w/v

Measured active content

IDENTITY, WHAT IT IS

MATCH

Confirmed

Retention-time match vs. same-day reference standard

CHROMATOGRAM

HPLC-UV

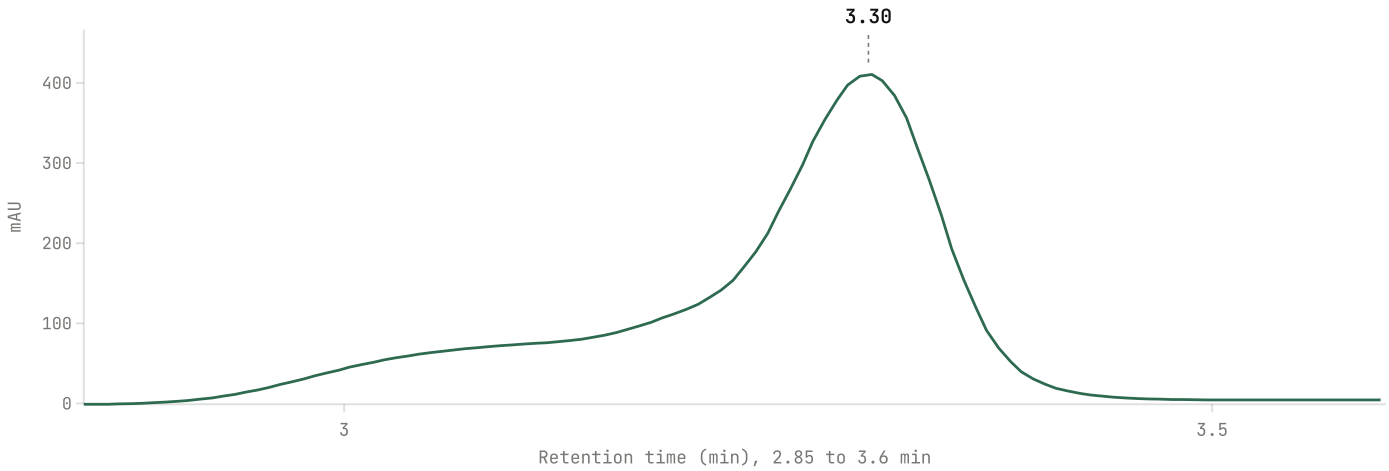

● 3.30 min, Benzyl Alcohol

ANALYST COMMENTS

Clear, colorless aqueous solution, blue-cap multi-dose vial, received sealed.

ANALYST SIGNATURE

Max Barrett
Lab Director, PuriLab Analytical
Analysis date: October 12, 2026

VERIFICATION CODE

BAC-G3XQ-JAJQ

Verify at purilab.org/verify/BAC-G3XQ-JAJQ

SCAN TO VERIFY

BAC-G3XQ-JAJQ

Results apply solely to the sample as received and are not representative of any larger lot, batch, or production run. Findings are limited to the analytes stated above. PuriLab Analytical is an independent testing laboratory, is not CLIA certified or ISO 17025 accredited, does not sell or distribute any substance, and makes no representation as to the safety, legality, or fitness of any material for any use.