



TIMELINE

ORDERED

October 9, 2026

RECEIVED

October 12, 2026

ANALYZED

October 12, 2026

SAMPLE

NAME

Bacteriostatic Water 10 mL

EXPECTED

Benzyl Alcohol (preservative)

AMOUNT

1 vial, aqueous solution, multi-dose 10 mL, sealed

TESTING

CLIENT

Investigate Peptides

TEST TYPE

Preservative identity & content determination

METHOD

HPLC-UV

CONTENT, HOW MUCH IS IN IT

0.91% w/v

Measured active content

IDENTITY, WHAT IT IS


MATCH

Confirmed

Retention-time match vs. same-day reference standard

CHROMATOGRAM

HPLC-UV

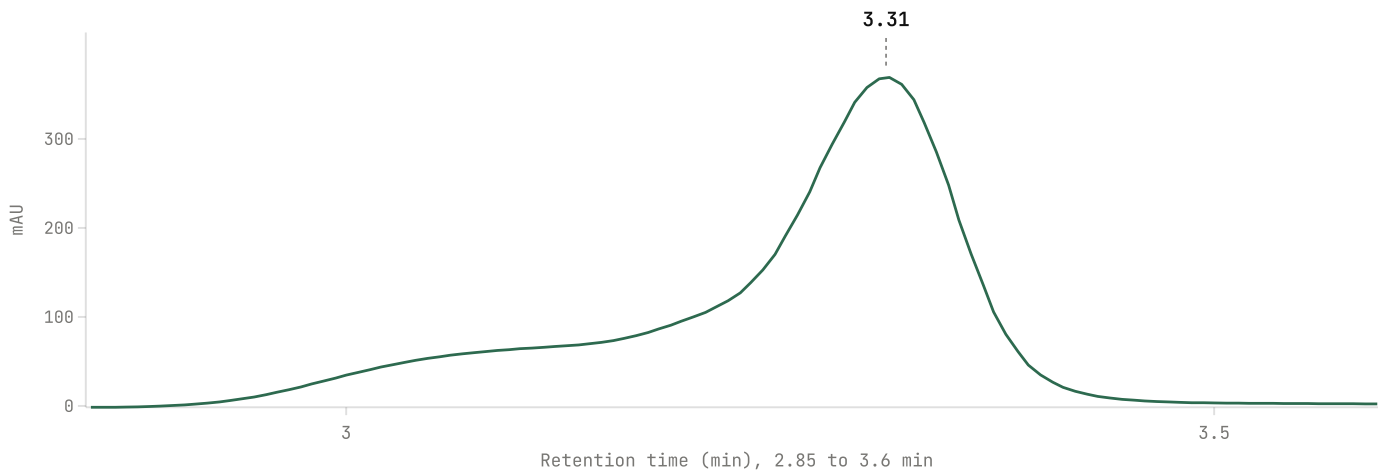

- 3.31 min, Benzyl Alcohol

ANALYST COMMENTS

Clear, colorless aqueous solution, white-cap multi-dose vial, received sealed.

ANALYST SIGNATURE

Max Barrett

Lab Director, PuriLab Analytical

Analysis date: October 12, 2026

VERIFICATION CODE

BAC-PJFD-HC72

Verify at purilab.org/verify/BAC-PJFD-HC72

SCAN TO VERIFY



BAC-PJFD-HC72

Results apply solely to the sample as received and are not representative of any larger lot, batch, or production run. Findings are limited to the analytes stated above. PuriLab Analytical is an independent testing laboratory, is not CLIA certified or ISO 17025 accredited, does not sell or distribute any substance, and makes no representation as to the safety, legality, or fitness of any material for any use.