



TIMELINE

ORDERED

October 10, 2026

RECEIVED

October 14, 2026

ANALYZED

October 15, 2026

SAMPLE

NAME

Bacteriostatic Water 3 mL

EXPECTED

Benzyl Alcohol (preservative)

AMOUNT

1 vial, aqueous solution, multi-dose 3 mL, sealed

TESTING

CLIENT

ATP Creative Labs

TEST TYPE

Preservative identity & content determination

METHOD

HPLC-UV

CONTENT, HOW MUCH IS IN IT

0.88% w/v

Measured active content

IDENTITY, WHAT IT IS


MATCH

Confirmed

Retention-time match vs. same-day reference standard

CHROMATOGRAM

HPLC-UV

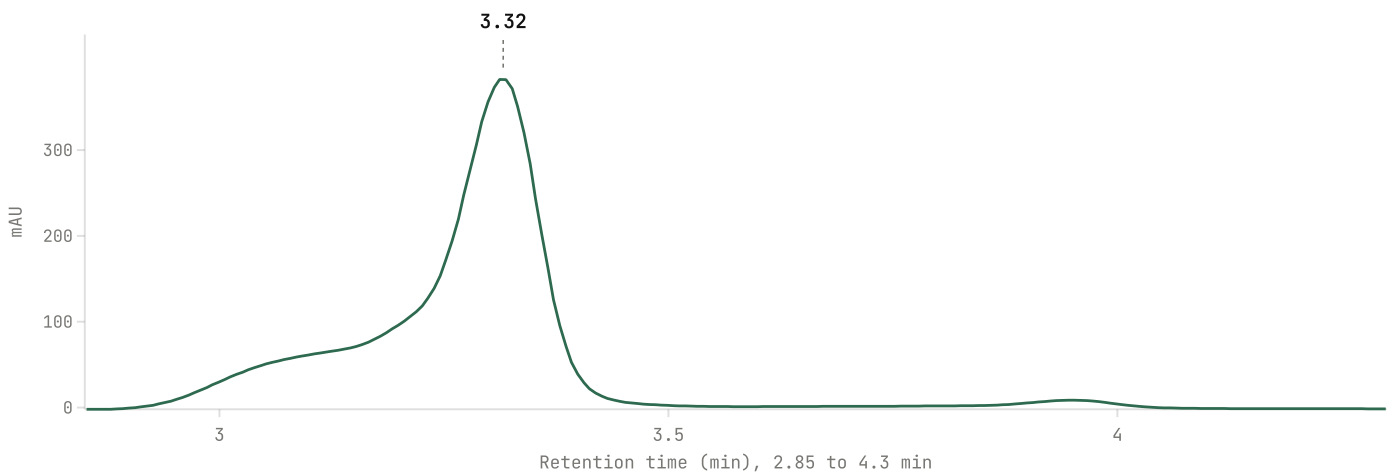

- 3.32 min, Benzyl Alcohol

ANALYST COMMENTS

Clear, colorless aqueous solution, blue-cap multi-dose vial, received sealed.

ANALYST SIGNATURE

Max Barrett

Lab Director, PuriLab Analytical

Analysis date: October 15, 2026

VERIFICATION CODE

BAC-54U3-9BDE

Verify at purilab.org/verify/BAC-54U3-9BDE

SCAN TO VERIFY



BAC-54U3-9BDE

Results apply solely to the sample as received and are not representative of any larger lot, batch, or production run. Findings are limited to the analytes stated above. PuriLab Analytical is an independent testing laboratory, is not CLIA certified or ISO 17025 accredited, does not sell or distribute any substance, and makes no representation as to the safety, legality, or fitness of any material for any use.