



TIMELINE

ORDERED

October 17, 2026

RECEIVED

October 22, 2026

ANALYZED

October 23, 2026

SAMPLE

NAME

Bacteriostatic Water 3 mL

EXPECTED

Benzyl Alcohol (preservative)

AMOUNT

1 vial, aqueous solution, multi-dose 3 mL, sealed

TESTING

CLIENT

Lavantis Labs

TEST TYPE

Preservative identity & content determination, pH

METHOD

HPLC-UV

CONTENT, HOW MUCH IS IN IT

0.95% w/v

Label claim: 0.9% w/v (USP)

IDENTITY, WHAT IT IS

Confirmed

Retention-time match vs. same-day reference standard

MATCH


PH

pH electrode, measured October 23, 2026

5.12

CHROMATOGRAM

HPLC-UV

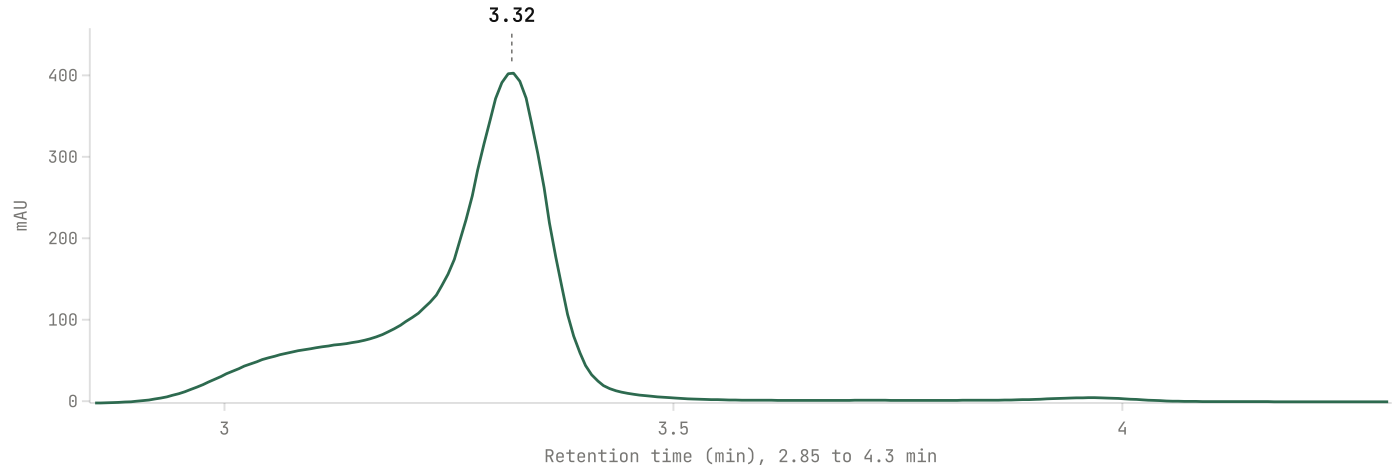

● 3.32 min, Benzyl Alcohol

ANALYST COMMENTS

Clear, colorless aqueous solution, white-cap multi-dose vial, received sealed.

ANALYST SIGNATURE

Max Barrett

Lab Director, PuriLab Analytical

Analysis date: October 23, 2026

VERIFICATION CODE

BAC-INYQ-UUE6

Verify at purilab.org/verify/BAC-INYQ-UUE6

SCAN TO VERIFY



BAC-INYQ-UUE6

Results apply solely to the sample as received and are not representative of any larger lot, batch, or production run. Findings are limited to the analytes stated above. PuriLab Analytical is an independent testing laboratory, is not CLIA certified or ISO 17025 accredited, does not sell or distribute any substance, and makes no representation as to the safety, legality, or fitness of any material for any use.