



TIMELINE	SAMPLE	TESTING
ORDERED	NAME	CLIENT
October 28, 2026	Bacteriostatic Water 3 mL	Bakersfield Aminos
RECEIVED	EXPECTED	TEST TYPE
October 29, 2026	Benzyl Alcohol (preservative)	Preservative identity & content determination, pH
ANALYZED	AMOUNT	METHOD
October 30, 2026	1 vial, aqueous solution, multi-dose 3 mL, sealed	HPLC-UV

CONTENT, HOW MUCH IS IN IT

0.97% w/v

Label claim: 0.9% w/v

IDENTITY, WHAT IT IS

MATCH

Confirmed

Retention-time and UV spectrum match vs. benzyl alcohol reference standard


PH

pH electrode, measured October 29, 2026

6.63

CHROMATOGRAM

HPLC-UV

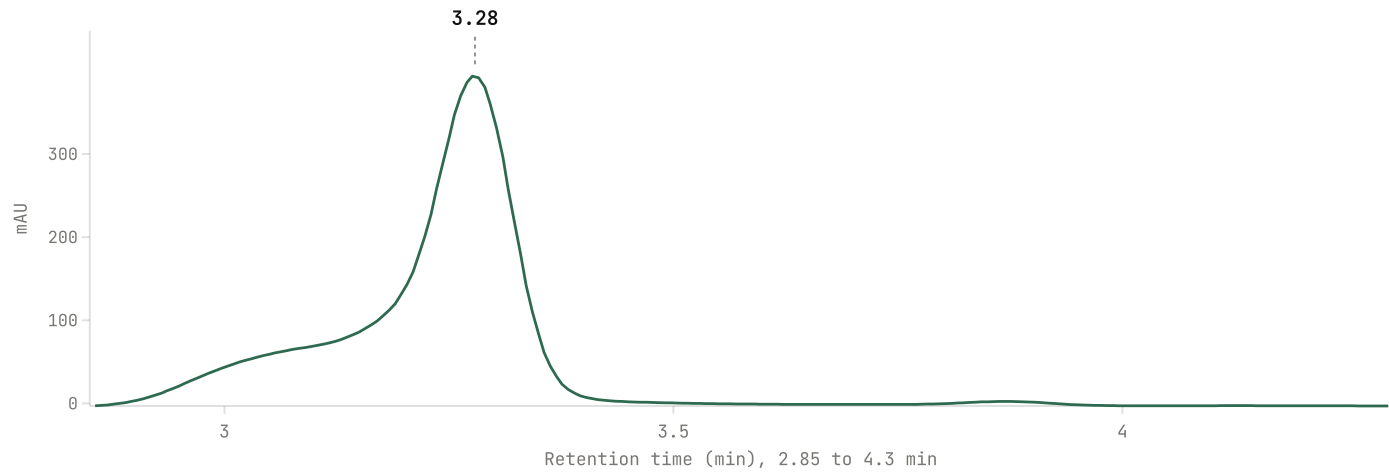

● 3.28 min, Benzyl Alcohol

ANALYST COMMENTS

Clear, colorless aqueous solution, white-cap multi-dose vial, received sealed.

ANALYST SIGNATURE

Max Barrett

Lab Director, PuriLab Analytical

Analysis date: October 30, 2026

VERIFICATION CODE

BAC-RQ6A-Y4NB

Verify at puriLab.org/verify/BAC-RQ6A-Y4NB

SCAN TO VERIFY



BAC-RQ6A-Y4NB

Results apply solely to the sample as received and are not representative of any larger lot, batch, or production run. Findings are limited to the analytes stated above. PuriLab Analytical is an independent testing laboratory, is not CLIA certified or ISO 17025 accredited, does not sell or distribute any substance, and makes no representation as to the safety, legality, or fitness of any material for any use.