



TIMELINE

ORDERED

October 26, 2026

RECEIVED

October 29, 2026

ANALYZED

October 30, 2026

SAMPLE

NAME

Bacteriostatic Water 3 mL

EXPECTED

Benzyl Alcohol (preservative)

AMOUNT

1 vial, aqueous solution, multi-dose 3 mL, sealed

TESTING

CLIENT

TVP

TEST TYPE

Preservative identity & content determination, pH

METHOD

HPLC-UV

CONTENT, HOW MUCH IS IN IT

0.66% w/v

Label claim: 0.9% w/v

IDENTITY, WHAT IT IS

MATCH

Confirmed

Retention-time and UV spectrum match vs. benzyl alcohol reference standard


PH

pH electrode, measured October 29, 2026

6.16

CHROMATOGRAM

HPLC-UV

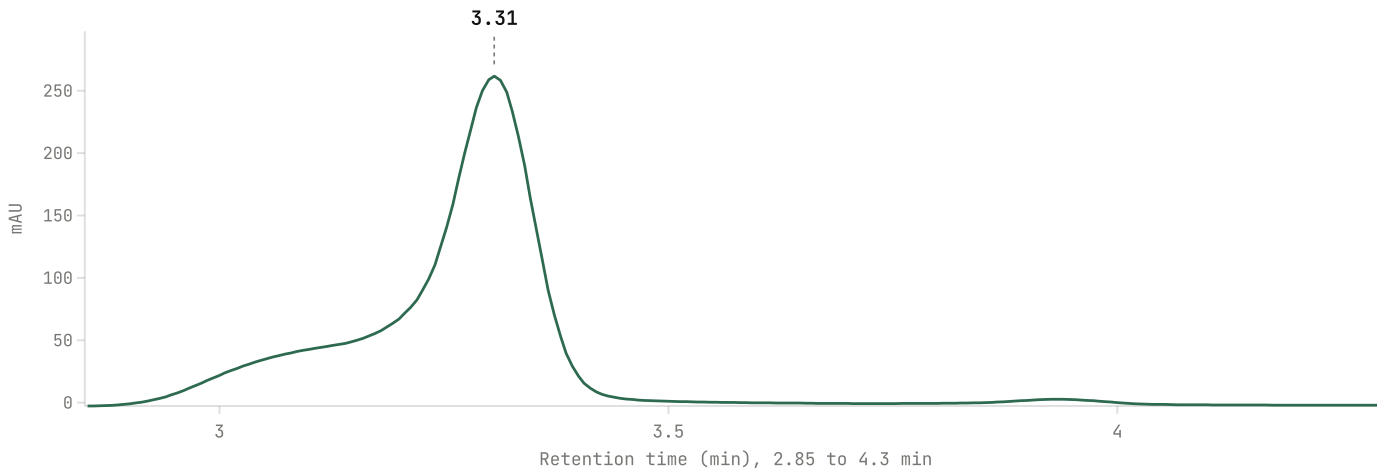

● 3.31 min, Benzyl Alcohol

ANALYST COMMENTS

Clear, colorless aqueous solution, white-cap multi-dose vial, received sealed.

ANALYST SIGNATURE

Max Barrett

Lab Director, PuriLab Analytical

Analysis date: October 30, 2026

VERIFICATION CODE

BAC-27X5-Y00K

Verify at purilab.org/verify/BAC-27X5-Y00K

SCAN TO VERIFY



BAC-27X5-Y00K

Results apply solely to the sample as received and are not representative of any larger lot, batch, or production run. Findings are limited to the analytes stated above. PuriLab Analytical is an independent testing laboratory, is not CLIA certified or ISO 17025 accredited, does not sell or distribute any substance, and makes no representation as to the safety, legality, or fitness of any material for any use.