CERTIFICATE OF ANALYSIS

PuriLab Analytical

Bacteriostatic Water 3 mL

BAC-2026-022 Lot NOT PROVIDED Analyzed November 5, 2026



TIMELINE

ORDERED
October 29, 2026

RECEIVED
November 4, 2026

ANALYZED
November 5, 2026

SAMPLE

NAME
Bacteriostatic Water 3 mL

EXPECTED
Benzyl Alcohol (preservative)

AMOUNT
1 vial, aqueous solution, multi-dose 3 mL, sealed

TESTING

CLIENT
New Wave Aminos

TEST TYPE
Preservative identity & content determination, pH, fentanyl

METHOD
HPLC-UV

CONTENT

0.94% w/v

Label claim: Not stated

IDENTITY — MATCH

Confirmed

Retention-time and UV spectrum match vs. benzyl alcohol reference standard

pH

5.85

USP range 4.5 to 7.0


FENTANYL

NOT DETECTED

Screening cutoff 20 ng/mL

CHROMATOGRAM

HPLC-UV

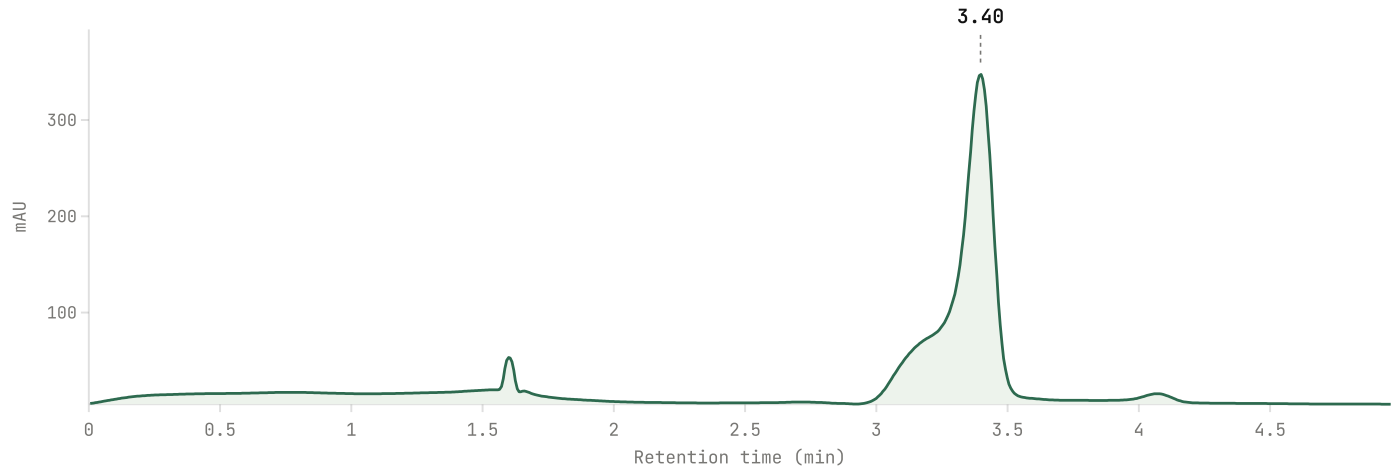

● 3.40 min, Benzyl Alcohol

ANALYST COMMENTS

Clear, colorless aqueous solution, black flip-cap multi-dose vial, received sealed.

ANALYST SIGNATURE

Max Barrett
Lab Director, PuriLab Analytical
Analysis date: November 5, 2026

VERIFICATION CODE

BAC-GSTT-92RC

Verify at purilab.org/verify/BAC-GSTT-92RC

SCAN TO VERIFY

BAC-GSTT-92RC

Results apply solely to the sample as received and are not representative of any larger lot, batch, or production run. Findings are limited to the analytes stated above. PuriLab Analytical is an independent testing laboratory, is not CLIA certified or ISO 17025 accredited, does not sell or distribute any substance, and makes no representation as to the safety, legality, or fitness of any material for any use.