CERTIFICATE OF ANALYSIS

PuriLab Analytical

Bacteriostatic Water 10 mL

BAC-2026-024 Lot CHL10262604 Analyzed November 5, 2026



TIMELINE

ORDERED
October 30, 2026

RECEIVED
November 3, 2026

ANALYZED
November 5, 2026

SAMPLE

NAME
Bacteriostatic Water 10 mL

EXPECTED
Benzyl Alcohol (preservative)

AMOUNT
1 vial, aqueous solution, multi-dose 10 mL, sealed

TESTING

CLIENT
Comfi Home Labs LLC

TEST TYPE
Preservative identity & content determination, pH

METHOD
HPLC-UV

CONTENT, HOW MUCH IS IN IT

0.91% w/v

Label claim: Not stated

IDENTITY, WHAT IT IS

MATCH

Confirmed

Retention-time and UV spectrum match vs. benzyl alcohol reference standard


pH

5.94

USP range 4.5 to 7.0

CHROMATOGRAM

HPLC-UV

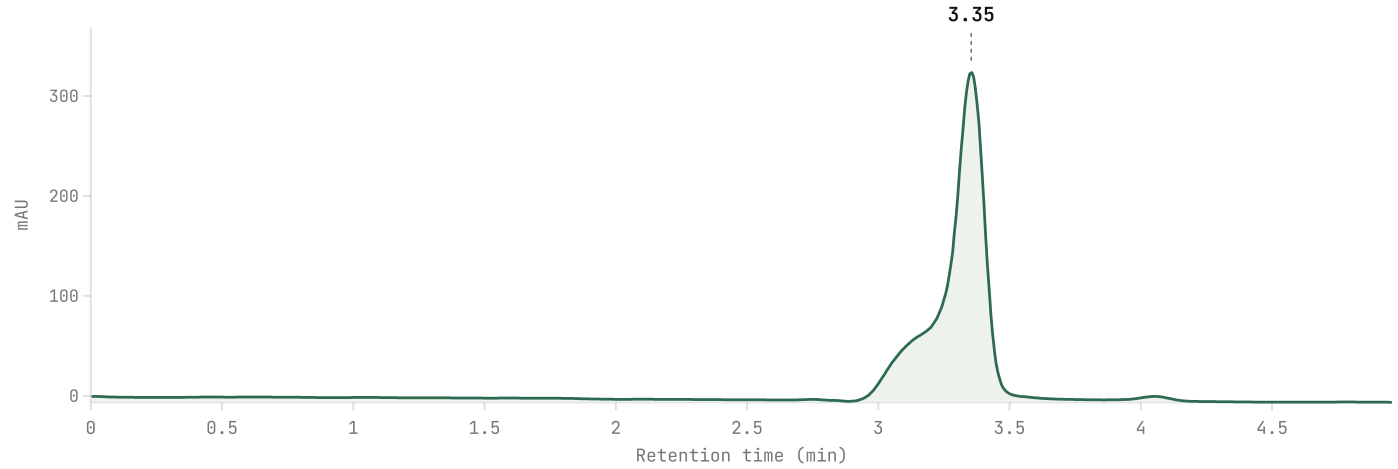

● 3.35 min, Benzyl Alcohol

ANALYST COMMENTS

Clear, colorless aqueous solution, blue flip-cap multi-dose vial, received sealed.

ANALYST SIGNATURE

Max Barrett
Lab Director, PuriLab Analytical
Analysis date: November 5, 2026

VERIFICATION CODE

BAC-M67Z-78ZW

Verify at purilab.org/verify/BAC-M67Z-78ZW

SCAN TO VERIFY

BAC-M67Z-78ZW

Results apply solely to the sample as received and are not representative of any larger lot, batch, or production run. Findings are limited to the analytes stated above. PuriLab Analytical is an independent testing laboratory, is not CLIA certified or ISO 17025 accredited, does not sell or distribute any substance, and makes no representation as to the safety, legality, or fitness of any material for any use.