CERTIFICATE OF ANALYSIS

PuriLab Analytical

Bacteriostatic Water 10 mL

BAC-2026-026 Lot NOT PROVIDED Analyzed November 5, 2026



TIMELINE

ORDERED
November 1, 2026

RECEIVED
November 5, 2026

ANALYZED
November 5, 2026

SAMPLE

NAME
Bacteriostatic Water 10 mL

EXPECTED
Benzyl Alcohol (preservative)

AMOUNT
1 vial, aqueous solution, multi-dose 10 mL, sealed

TESTING

CLIENT
Vantage

TEST TYPE
Preservative identity & content determination, pH

METHOD
HPLC-UV

GROUP TEST

VIALS TESTED
1 vial, shared result

CONTRIBUTORS
9 people

SHARED BY
Pretty Pep Co, Branded Blends LLC, Aesthelix Bloom, Peberekspressen, Put Together(ish) Peps, PEP PLUG UK, WHresearch, Down Under Research, Nexylab

CONTENT, HOW MUCH IS IN IT

0.92% w/v

Label claim: 0.9% w/v

IDENTITY, WHAT IT IS

MATCH

Confirmed

Retention-time and UV spectrum match vs. benzyl alcohol reference standard


pH

6.35

USP range 4.5 to 7.0

CHROMATOGRAM

HPLC-UV

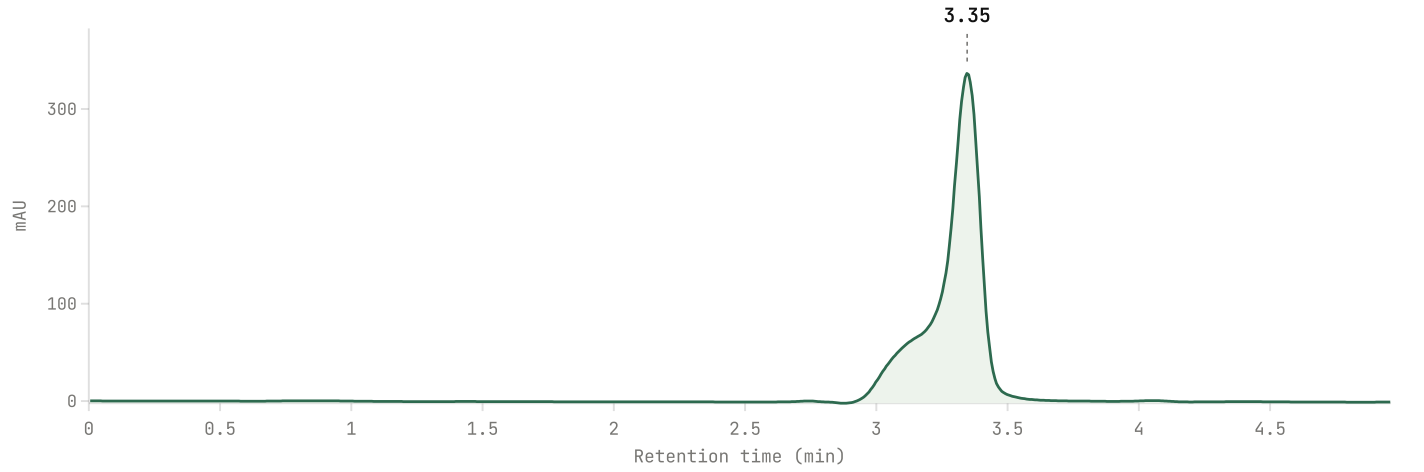

● 3.35 min, Benzyl Alcohol

ANALYST COMMENTS

Clear, colorless aqueous solution, blue flip-cap multi-dose vial, received sealed.

ANALYST SIGNATURE

Max Barrett
Lab Director, PuriLab Analytical
Analysis date: November 5, 2026

VERIFICATION CODE

BAC-37Z9-TES9

Verify at purilab.org/verify/BAC-37Z9-TES9

SCAN TO VERIFY

BAC-37Z9-TES9

Results apply solely to the sample as received and are not representative of any larger lot, batch, or production run. Findings are limited to the analytes stated above. PuriLab Analytical is an independent testing laboratory, is not CLIA certified or ISO 17025 accredited, does not sell or distribute any substance, and makes no representation as to the safety, legality, or fitness of any material for any use.