CERTIFICATE OF ANALYSIS

PuriLab Analytical

Wolverine 20 mg

BT-2026-023 Lot NOT PROVIDED Analyzed November 11, 2026



TIMELINE

ORDERED
October 29, 2026

RECEIVED
November 4, 2026

ANALYZED
November 11, 2026

SAMPLE

NAME
Wolverine 20 mg

EXPECTED
Wolverine blend (BPC-157, TB-500)

AMOUNT
2 vials (same product, conformity), lyophilized powder

TESTING

CLIENT
New Wave Aminos

TEST TYPE
Content & purity, fentanyl, conformity

METHOD
HPLC-UV

CONTENT, HOW MUCH IS IN IT

BPC-157, bottle 1	19.63 mg	Label claim: 10 mg
TB-500 (full-length TB4), bottle 1	9.80 mg	Label claim: 10 mg
BPC-157, bottle 2	24.39 mg	Label claim: 10 mg
TB-500, bottle 2	Not detected	Label claim: 10 mg

PURITY, HOW CLEAN IT IS

99.7% (bottle 1)

Bottle 1, HPLC-UV peak area. Measured, not estimated. Purity is calculated from the full chromatogram shown above.

FENTANYL

NOT DETECTED

Screening cutoff 20 ng/mL


CONFORMITY — DOES NOT CONFORM

The bottles do not match. Bottle 1 contains BPC-157 and full-length TB-500 (TB4); bottle 2 contains BPC-157 only, with no TB-500 detected (full-length or fragment, detection limit about 0.05 mg). No average is given because the bottles differ. Solid trace is bottle 1, dashed trace is bottle 2. Bottle 1 received November 4, 2026, analyzed November 6, 2026. Bottle 2 received November 10, 2026, analyzed November 11, 2026.

Vial	Content	Purity
Bottle 1	BPC-157 19.63 mg / TB-500 9.80 mg	99.7%
Bottle 2	BPC-157 24.39 mg / TB-500 not detected	99.4%

CHROMATOGRAM

HPLC-UV

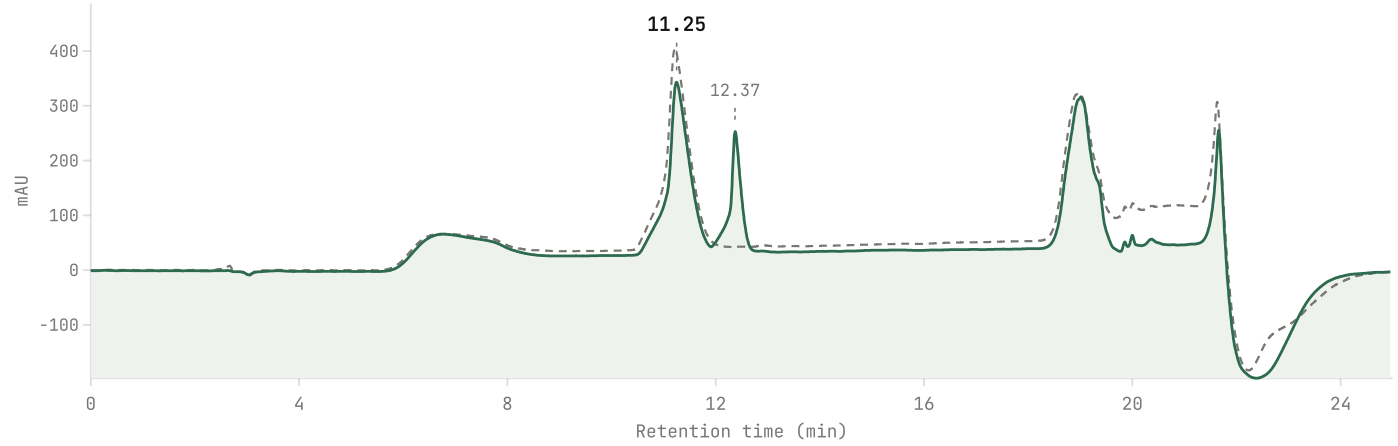

● 11.25 min, BPC-157, 71.6% ● 12.37 min, TB-500 (full-length TB4), 28.1% --- Bottle 2 (TB-500 not detected)

ANALYST COMMENTS

White lyophilized powder, black-cap vials, received sealed.

ANALYST SIGNATURE

Max Barrett
Lab Director, PuriLab Analytical
Analysis date: November 11, 2026

VERIFICATION CODE

BT-VSH1-WYYO

Verify at purilab.org/verify/BT-VSH1-WYYO

SCAN TO VERIFY

BT-VSH1-WYYO

Results apply solely to the sample as received and are not representative of any larger lot, batch, or production run. Findings are limited to the analytes stated above. PuriLab Analytical is an independent testing laboratory, is not CLIA certified or ISO 17025 accredited, does not sell or distribute any substance, and makes no representation as to the safety, legality, or fitness of any material for any use.