CERTIFICATE OF ANALYSIS

PuriLab Analytical

GHK-Cu 100 mg / KPV 10 mg

GH-2026-007 Lot NOT PROVIDED Analyzed November 1, 2026



TIMELINE

ORDERED
October 26, 2026

RECEIVED
October 28, 2026

ANALYZED
November 1, 2026

SAMPLE

NAME
GHK-Cu 100 mg / KPV 10 mg

EXPECTED
GHK-Cu + KPV blend

AMOUNT
1 vial, lyophilized powder

TESTING

CLIENT
4Ever Research

TEST TYPE
Content & purity

METHOD
HPLC-UV

CONTENT, HOW MUCH IS IN IT

GHK-Cu	98.9 mg	Label claim: 100 mg
KPV	9.7 mg	Label claim: 10 mg


PURITY, HOW CLEAN IT IS

>99%

GHK-Cu + KPV, HPLC-UV peak area

CHROMATOGRAM

HPLC-UV

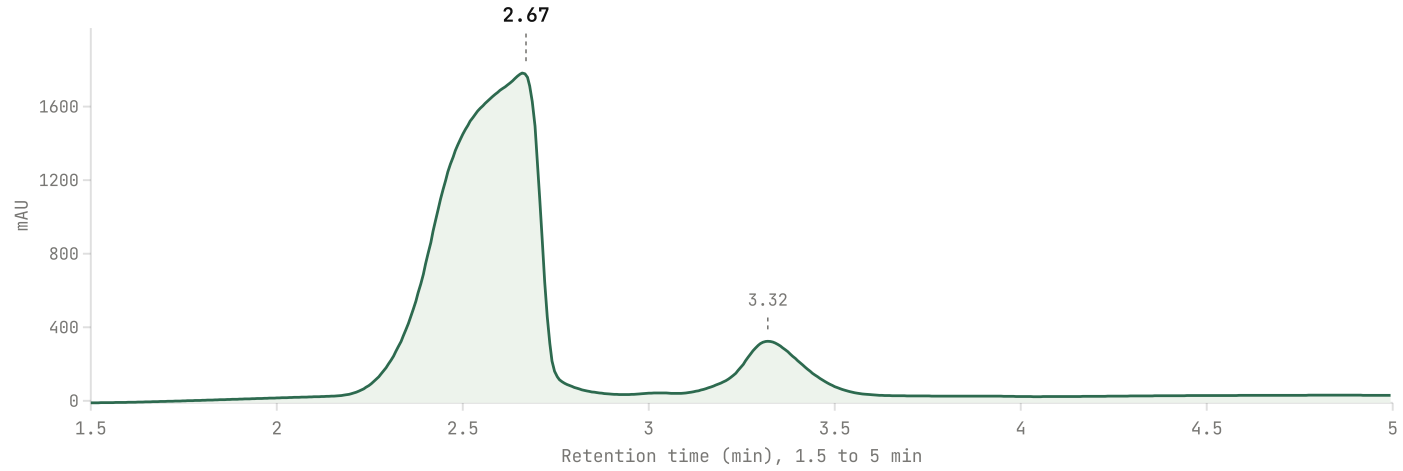

● 2.67 min, GHK-Cu ● 3.32 min, KPV

ANALYST COMMENTS

Light blue lyophilized powder, blue-cap vial, received sealed.

ANALYST SIGNATURE

Max Barrett
Lab Director, PuriLab Analytical
Analysis date: November 1, 2026

VERIFICATION CODE

GH-70Z7-GQJP

Verify at purilab.org/verify/GH-70Z7-GQJP

SCAN TO VERIFY

GH-70Z7-GQJP

Results apply solely to the sample as received and are not representative of any larger lot, batch, or production run. Findings are limited to the analytes stated above. PuriLab Analytical is an independent testing laboratory, is not CLIA certified or ISO 17025 accredited, does not sell or distribute any substance, and makes no representation as to the safety, legality, or fitness of any material for any use.