CERTIFICATE OF ANALYSIS

PuriLab Analytical

Retatrutide 10 mg

RT-2026-093 Lot LUMI593-A17 Analyzed November 7, 2026



TIMELINE

ORDERED
November 3, 2026

RECEIVED
November 6, 2026

ANALYZED
November 7, 2026

SAMPLE

NAME
Retatrutide 10 mg

EXPECTED
Retatrutide

AMOUNT
1 vial, lyophilized powder

TESTING

CLIENT
Aguila Aminos

TEST TYPE
Content & purity, fentanyl

METHOD
HPLC-UV

CONTENT, HOW MUCH IS IN IT

12.27 mg

Label claim: 10 mg

PURITY, HOW CLEAN IT IS

99.9%

by HPLC-UV peak area, system peaks excluded


FENTANYL

NOT DETECTED

Screening cutoff 20 ng/mL

CHROMATOGRAM

HPLC-UV

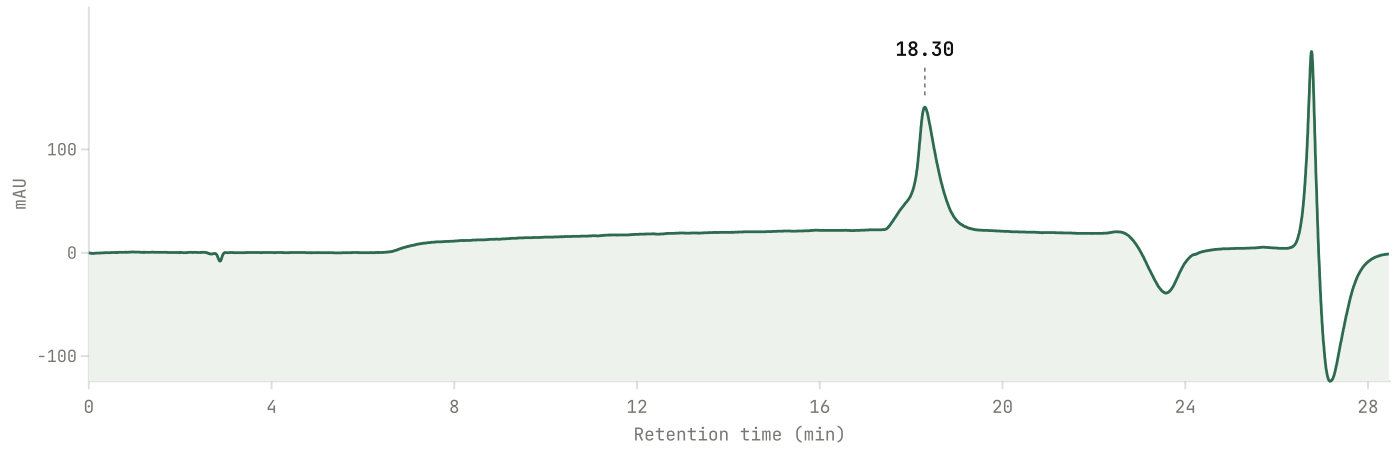

- 18.30 min, Retatrutide, 99.9%

ANALYST COMMENTS

White lyophilized powder, blue-cap vial, received sealed.

ANALYST SIGNATURE

Max Barrett
Lab Director, PuriLab Analytical
Analysis date: November 7, 2026

VERIFICATION CODE

RT-1RJ2-8Q2Y

Verify at purilab.org/verify/RT-1RJ2-8Q2Y

SCAN TO VERIFY

RT-1RJ2-8Q2Y

Results apply solely to the sample as received and are not representative of any larger lot, batch, or production run. Findings are limited to the analytes stated above. PuriLab Analytical is an independent testing laboratory, is not CLIA certified or ISO 17025 accredited, does not sell or distribute any substance, and makes no representation as to the safety, legality, or fitness of any material for any use.