CERTIFICATE OF ANALYSIS

PuriLab Analytical

Retatrutide 30 mg

RT-2026-097 Lot PED261015001 Analyzed November 7, 2026



TIMELINE

ORDERED
November 2, 2026

RECEIVED
November 6, 2026

ANALYZED
November 7, 2026

SAMPLE

NAME
Retatrutide 30 mg

EXPECTED
Retatrutide

AMOUNT
1 vial, lyophilized powder

TESTING

CLIENT
Anonymous

TEST TYPE
Content & purity

METHOD
HPLC-UV

CONTENT, HOW MUCH IS IN IT

35.06 mg

Label claim: 30 mg


PURITY, HOW CLEAN IT IS

99.9%

by HPLC-UV peak area, system peaks excluded

CHROMATOGRAM

HPLC-UV

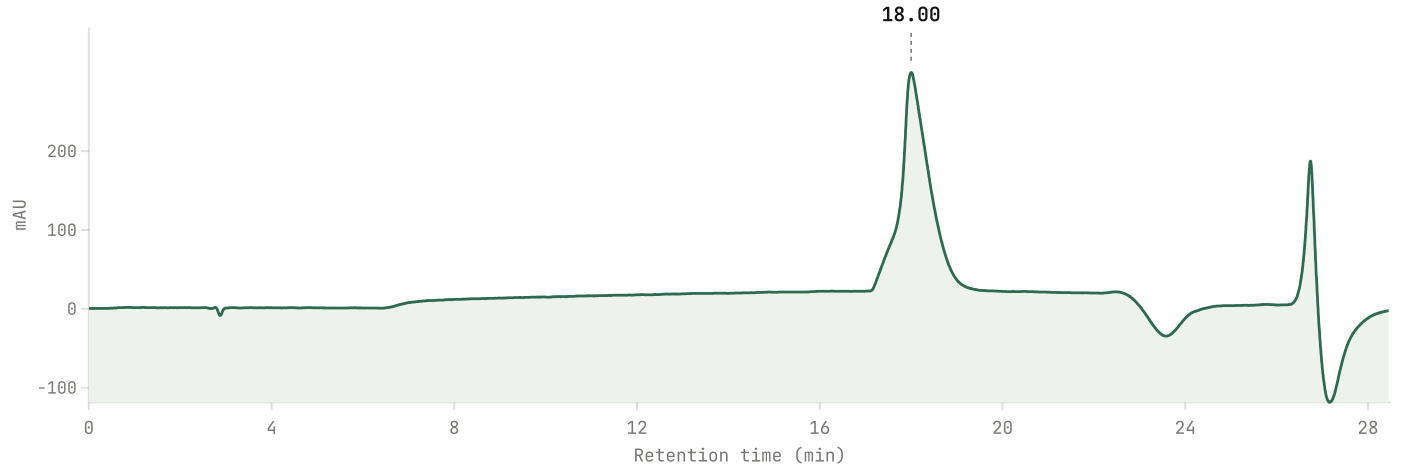

- 18.00 min, Retatrutide, 99.9%

ANALYST COMMENTS

White lyophilized powder, blue-cap vial, received sealed. Unlabeled vial; label claim taken from the order.

ANALYST SIGNATURE

Max Barrett
Lab Director, PuriLab Analytical
Analysis date: November 7, 2026

VERIFICATION CODE

RT-26DH-3XK5

Verify at purilab.org/verify/RT-26DH-3XK5

SCAN TO VERIFY

RT-26DH-3XK5

Results apply solely to the sample as received and are not representative of any larger lot, batch, or production run. Findings are limited to the analytes stated above. PuriLab Analytical is an independent testing laboratory, is not CLIA certified or ISO 17025 accredited, does not sell or distribute any substance, and makes no representation as to the safety, legality, or fitness of any material for any use.