CERTIFICATE OF ANALYSIS

PuriLab Analytical

VB-RT3 15 mg

RT-2026-149 Lot 1126915 Analyzed November 20, 2026



TIMELINE

ORDERED
November 16, 2026

RECEIVED
November 19, 2026

ANALYZED
November 20, 2026

SAMPLE

NAME
VB-RT3 15 mg

EXPECTED
VB-RT3

AMOUNT
1 vial, lyophilized powder

TESTING

CLIENT
Volunteer Bio

TEST TYPE
Content & purity

METHOD
HPLC-UV

CONTENT, HOW MUCH IS IN IT

15.46 mg

Label claim: 15 mg


PURITY, HOW CLEAN IT IS

>99.9%

Measured, not estimated. Purity is calculated from the full chromatogram shown above, and no impurity peaks were detected above the reporting threshold. Results of 99.95% or higher are reported as >99.9%, as 100% purity cannot be demonstrated analytically.

CHROMATOGRAM

HPLC-UV

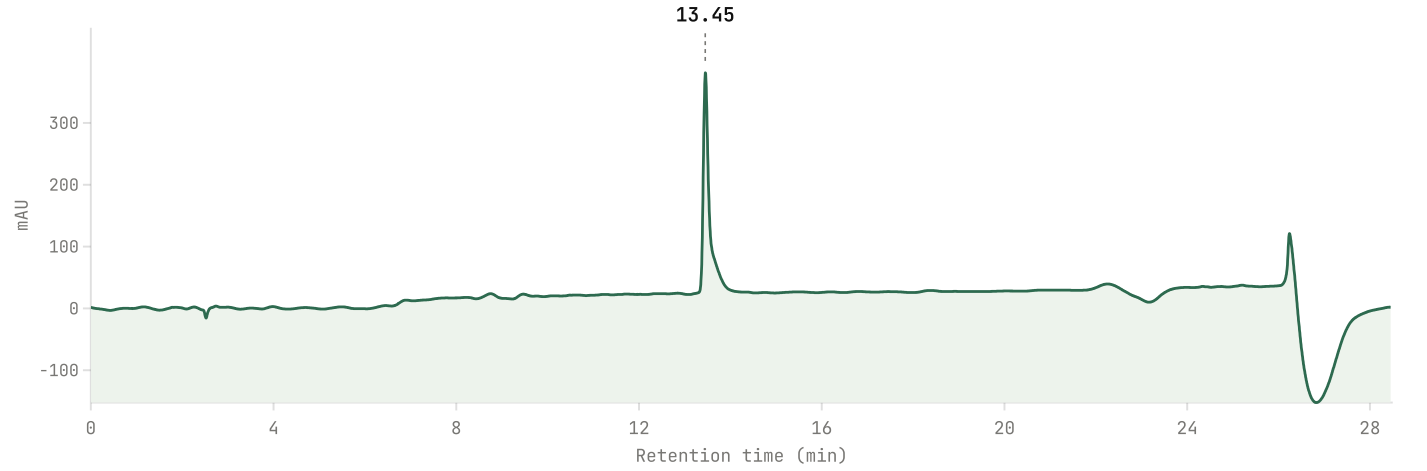

- 13.45 min, VB-RT3, >99.9%

ANALYST COMMENTS

White lyophilized powder, red flip-cap vial, received sealed.

ANALYST SIGNATURE

Max Barrett
Lab Director, PuriLab Analytical
Analysis date: November 20, 2026

VERIFICATION CODE

RT-E3NR-Y062

Verify at purilab.org/verify/RT-E3NR-Y062

SCAN TO VERIFY

RT-E3NR-Y062

Results apply solely to the sample as received and are not representative of any larger lot, batch, or production run. Findings are limited to the analytes stated above. PuriLab Analytical is an independent testing laboratory, is not CLIA certified or ISO 17025 accredited, does not sell or distribute any substance, and makes no representation as to the safety, legality, or fitness of any material for any use.