CERTIFICATE OF ANALYSIS

PuriLab Analytical

VB-RT3 10 mg

RT-2026-150 Lot 1126910 Analyzed November 20, 2026



TIMELINE	SAMPLE	TESTING
ORDERED	NAME	CLIENT
November 16, 2026	VB-RT3 10 mg	Volunteer Bio
RECEIVED	EXPECTED	TEST TYPE
November 19, 2026	VB-RT3	Content & purity
ANALYZED	AMOUNT	METHOD
November 20, 2026	1 vial, lyophilized powder	HPLC-UV

CONTENT, HOW MUCH IS IN IT

10.35 mg


Label claim: 10 mg

PURITY, HOW CLEAN IT IS

96.3%

Measured, not estimated. Purity is calculated from the full chromatogram shown above.

CHROMATOGRAM HPLC-UV

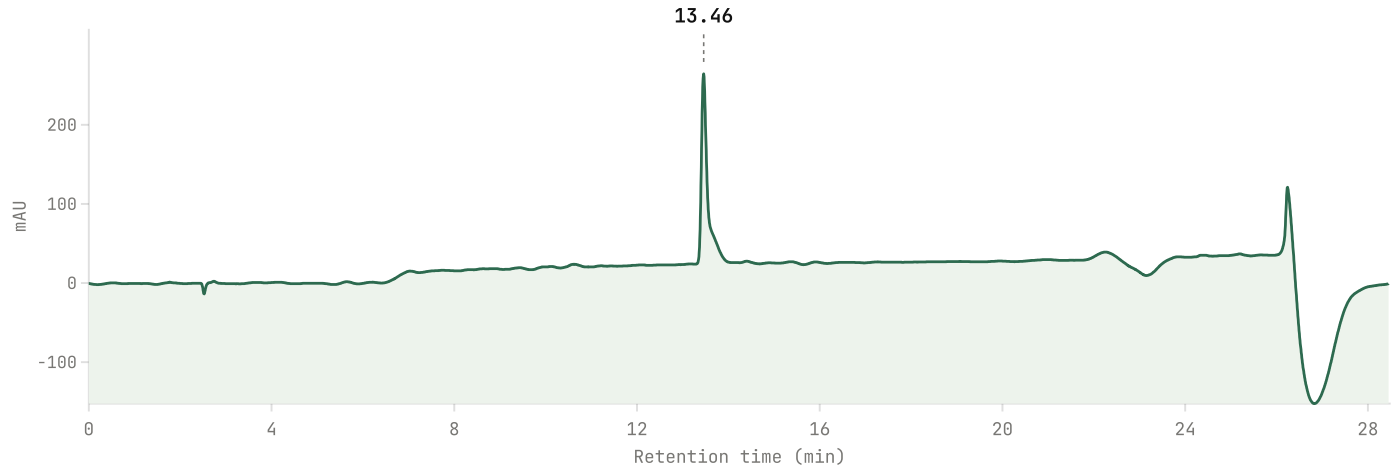

- 13.46 min, VB-RT3, 96.3%

ANALYST COMMENTS

White lyophilized powder, blue flip-cap vial, received sealed.

ANALYST SIGNATURE

Max Barrett
Lab Director, PuriLab Analytical
Analysis date: November 20, 2026

VERIFICATION CODE

RT-RJQO-72AP

Verify at purilab.org/verify/RT-RJQO-72AP

SCAN TO VERIFY

RT-RJQO-72AP

Results apply solely to the sample as received and are not representative of any larger lot, batch, or production run. Findings are limited to the analytes stated above. PuriLab Analytical is an independent testing laboratory, is not CLIA certified or ISO 17025 accredited, does not sell or distribute any substance, and makes no representation as to the safety, legality, or fitness of any material for any use.