CERTIFICATE OF ANALYSIS

PuriLab Analytical

SS-31 50 mg

SS-2026-006 Lot SYN-R8F9YAL Analyzed November 14, 2026



TIMELINE		SAMPLE		TESTING	
ORDERED	November 5, 2026	NAME	SS-31 50 mg	CLIENT	Synaptik Solutions
RECEIVED	November 13, 2026	EXPECTED	SS-31	TEST TYPE	Content & purity
ANALYZED	November 14, 2026	AMOUNT	1 vial, lyophilized powder	METHOD	HPLC-UV

CONTENT, HOW MUCH IS IN IT

54.66 mg

Label claim: 50 mg


PURITY, HOW CLEAN IT IS

99.8%

by HPLC-UV peak area, system peaks excluded

CHROMATOGRAM

HPLC-UV

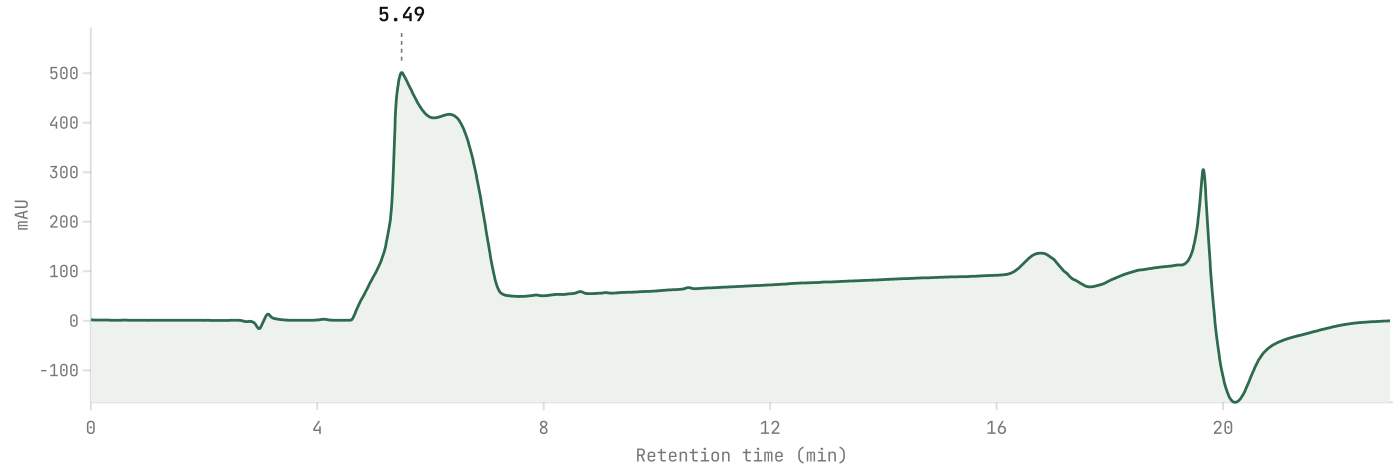

● 5.49 min, SS-31, 99.8%

ANALYST COMMENTS

White lyophilized powder, magenta-cap vial, received sealed.

ANALYST SIGNATURE

Max Barrett
Lab Director, PuriLab Analytical
Analysis date: November 14, 2026

VERIFICATION CODE

SS-30OV-ABQL

Verify at purilab.org/verify/SS-30OV-ABQL

SCAN TO VERIFY

SS-30OV-ABQL

Results apply solely to the sample as received and are not representative of any larger lot, batch, or production run. Findings are limited to the analytes stated above. PuriLab Analytical is an independent testing laboratory, is not CLIA certified or ISO 17025 accredited, does not sell or distribute any substance, and makes no representation as to the safety, legality, or fitness of any material for any use.