

Semax 10 mg

SX-2026-004 Lot PX-H6YFR9 Analyzed October 29, 2026



TIMELINE

ORDERED

October 26, 2026

RECEIVED

October 28, 2026

ANALYZED

October 29, 2026

SAMPLE

NAME

Semax 10 mg

EXPECTED

Semax

AMOUNT

1 vial, lyophilized powder

TESTING

CLIENT

Prime X Compounds

TEST TYPE

Content & purity

METHOD

HPLC-UV

CONTENT, HOW MUCH IS IN IT

10.76 mg

Label claim: 10 mg


PURITY, HOW CLEAN IT IS

>99.9%

by HPLC-UV peak area

CHROMATOGRAM

HPLC-UV

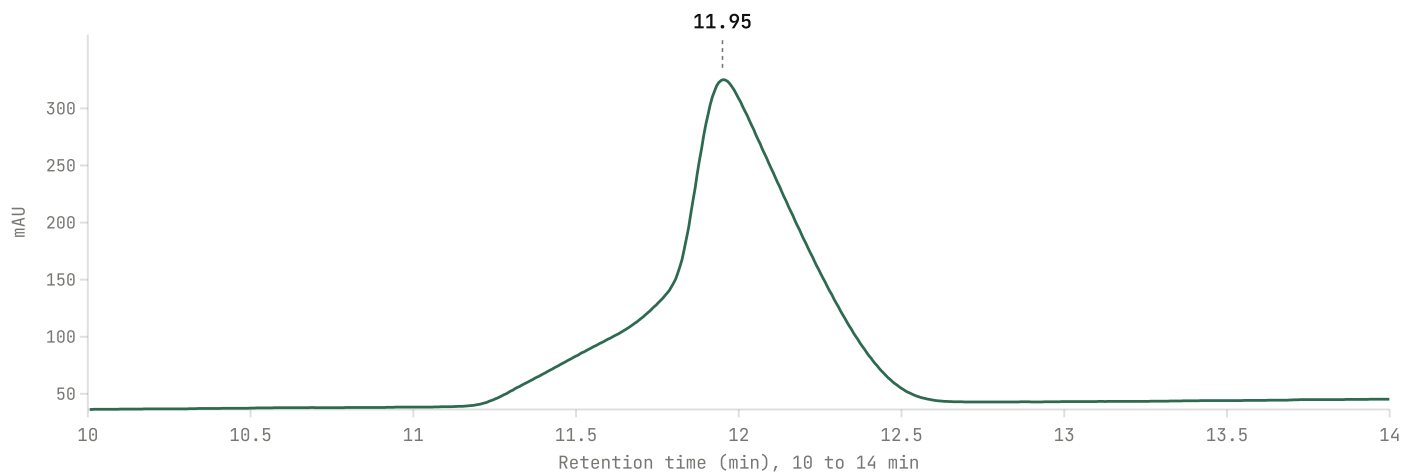

● 11.95 min, Semax, >99.9%

ANALYST COMMENTS

White lyophilized powder, blue-cap vial, received sealed.

ANALYST SIGNATURE

Max Barrett

Lab Director, PuriLab Analytical

Analysis date: October 29, 2026

VERIFICATION CODE

SX-BLY9-F4RAVerify at purilab.org/verify/SX-BLY9-F4RA

SCAN TO VERIFY



SX-BLY9-F4RA

Results apply solely to the sample as received and are not representative of any larger lot, batch, or production run. Findings are limited to the analytes stated above. PuriLab Analytical is an independent testing laboratory, is not CLIA certified or ISO 17025 accredited, does not sell or distribute any substance, and makes no representation as to the safety, legality, or fitness of any material for any use.