CERTIFICATE OF ANALYSIS

PuriLab Analytical

Semax + Selank 20 mg

SX-2026-005 Lot NOT PROVIDED Analyzed November 3, 2026



TIMELINE

ORDERED
October 29, 2026

RECEIVED
October 31, 2026

ANALYZED
November 3, 2026

SAMPLE

NAME
Semax + Selank 20 mg

EXPECTED
Semax + Selank

AMOUNT
1 vial, lyophilized powder

TESTING

CLIENT
4Ever Research

TEST TYPE
Content & purity

METHOD
HPLC-UV

CONTENT, HOW MUCH IS IN IT

Semax	13.92 mg	Label claim: 10 mg
Selank	14.90 mg	Label claim: 10 mg


PURITY, HOW CLEAN IT IS

99.1%

by HPLC-UV peak area, system peaks excluded


CHROMATOGRAMS

SEMAX — HPLC-UV

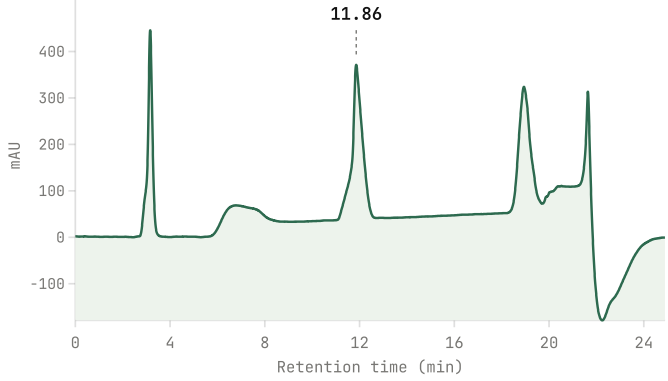

● 11.86 min, Semax

SELANK — HPLC-UV

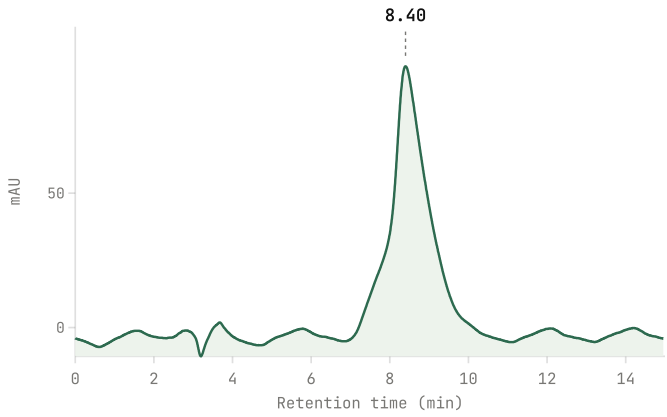

● 8.40 min, Selank

ANALYST COMMENTS

White lyophilized powder, clear-cap vial, received sealed.

ANALYST SIGNATURE

Max Barrett
Lab Director, PuriLab Analytical
Analysis date: November 3, 2026

VERIFICATION CODE

SX-HMUW-YJO3
Verify at purilab.org/verify/SX-HMUW-YJO3

SCAN TO VERIFY

SX-HMUW-YJO3

Results apply solely to the sample as received and are not representative of any larger lot, batch, or production run. Findings are limited to the analytes stated above. PuriLab Analytical is an independent testing laboratory, is not CLIA certified or ISO 17025 accredited, does not sell or distribute any substance, and makes no representation as to the safety, legality, or fitness of any material for any use.