CERTIFICATE OF ANALYSIS

PuriLab Analytical

XA10 10 mg

SX-2026-010 Lot XA10-1126-A01 Analyzed November 17, 2026



TIMELINE

ORDERED
November 10, 2026

RECEIVED
November 16, 2026

ANALYZED
November 17, 2026

SAMPLE

NAME
XA10 10 mg

EXPECTED
XA10

AMOUNT
1 vial, lyophilized powder

TESTING

CLIENT
Group Test A

TEST TYPE
Content & purity

METHOD
HPLC-UV

CONTENT, HOW MUCH IS IN IT

13.31 mg

Label claim: 10 mg


PURITY, HOW CLEAN IT IS

99.3%

by HPLC-UV peak area, system peaks excluded

CHROMATOGRAM

HPLC-UV

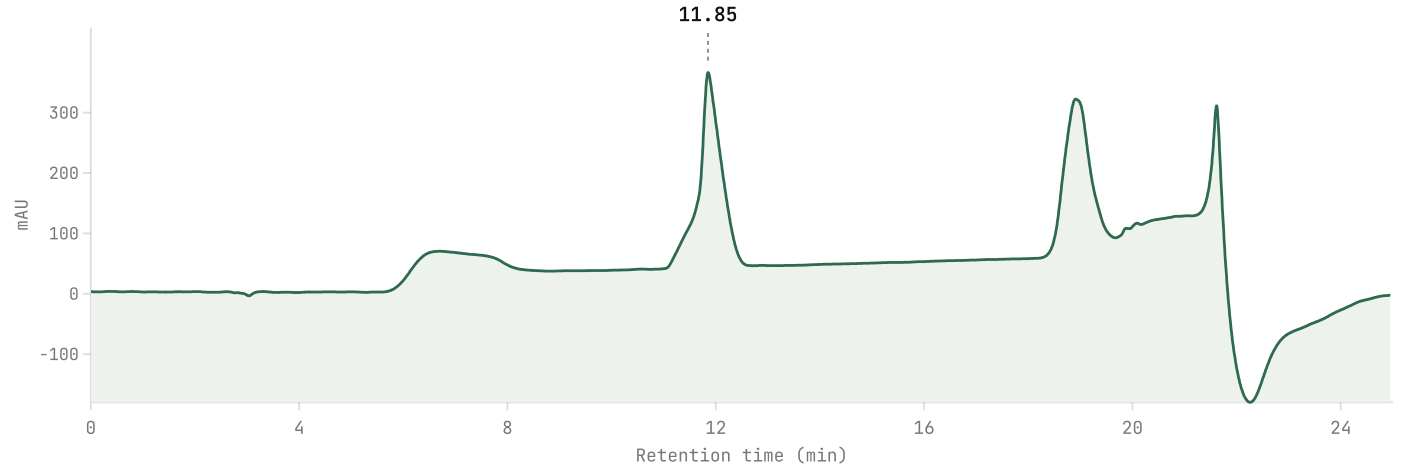

- 11.85 min, XA10, 99.3%

ANALYST COMMENTS

White lyophilized powder, black-cap vial, received sealed.

ANALYST SIGNATURE

Max Barrett
Lab Director, PuriLab Analytical
Analysis date: November 17, 2026

VERIFICATION CODE

SX-J9I0-ZKDQ

Verify at purilab.org/verify/SX-J9I0-ZKDQ

SCAN TO VERIFY

SX-J9I0-ZKDQ

Results apply solely to the sample as received and are not representative of any larger lot, batch, or production run. Findings are limited to the analytes stated above. PuriLab Analytical is an independent testing laboratory, is not CLIA certified or ISO 17025 accredited, does not sell or distribute any substance, and makes no representation as to the safety, legality, or fitness of any material for any use.